

Manuscripts received July 18, 2023; revised August 10, 2023; accepted August 12, 2023; Publish date: 25 September 2023
Digital Object Identifier (DOI): <https://doi.org/10.35882/teknokes.v16i3.609>
Copyright © 2023 by the authors. This work is an open-access article and licensed under a Creative Commons Attribution-ShareAlike 4.0 International License ([CC BY-SA 4.0](https://creativecommons.org/licenses/by-sa/4.0/))
How to cite: Rizky Dwi K, M. Prastawa Assalim Tetra Putra, Abdul Kholiq, Bedjo Utomo, Sumber, Triwiyanto and Yagnik Rathod, "IoT-Based Human Vital Sign Monitoring Tool Using Telegram Notifications (BPM and Respiration Rate Parameters) ", Jurnal Teknokes, vol. 16, no. 1, pp. 185–190, September. 2023.

IoT-Based Human Vital Sign Monitoring Tool Using Telegram Notifications

Rizky Dwi K¹, M. Prastawa Assalim Tetra Putra¹, Abdul Kholiq¹, Bedjo Utomo¹, Sumber¹, Triwiyanto¹ and Yagnik Rathod²

¹ Department of Electromedical Engineering, Health Polytechnic Ministry of Health Surabaya, Surabaya, Indonesia
² Department of Computer Engineering, Government Engineering College, Dahod, India

Corresponding author: Bedjo Utomo (e-mail: Bedjoutomo123@gmail.com).

"This work was supported in part by Department of Electromedical Engineering, Health Polytechnic Ministry of Health Surabaya"

ABSTRACT Vital signs play a crucial role in monitoring the progress of adult or pediatric patients during hospitalization, as they enable prompt detection of delayed recovery or adverse events. Vital signs are measured to obtain fundamental indicators of the patient's health status. The measurement of vital signs, including blood pressure, temperature, pulse, and respiratory rate, is the most common intervention in hospital medicine. Advanced monitoring systems combine clinical and technological aspects to deliver innovative healthcare outcomes. Remote patient monitoring systems are increasingly becoming the cornerstone of healthcare delivery, replacing traditional manual recording with computer and smartphone-based electronic recording as a versatile and innovative health monitoring system. This study aims to design a Vital Sign Monitoring Parameter BPM and RR tool with Notifications via the IoT-Based Telegram application. The tool enables the monitoring of vital signs, particularly BPM and RR, regardless of the patient's location and at any given time. This allows doctors, health workers, and patients to stay informed about their health condition. Real-time display of vital sign data is available through the TFT LCD screen, and the data from the screen can be accessed via Telegram. The Telegram application will send notifications in the event of abnormal patient conditions. MAX30100, a digital sensor for detecting breathing rate and heart rate, is utilized in this research. Furthermore, the data obtained shows errors that are within the allowable limits for each parameter. The difference between the heart rate readings and the respiratory rate values on the device and the patient monitor is 1.14% for heart rate and 0.84% for respiratory rate. This study indicates that it is time to monitor vital signs that can be seen remotely and have a system that is an inexpensive and easy-to-operate device for health workers without interfering with activities of daily living.

INDEX TERMS Smartband, Multiplexer, SEN0203, MLX90614, BPM, Temperature

I. INTRODUCTION

Vital signs are an essential component of monitoring the adult or child patient's progress during hospitalization, as they allow for the prompt detection of delayed recovery or adverse events. Vital signs are measured to obtain fundamental indicators of a patient's health status. The most common intervention performed in hospital medicine is a measurement of vital signs [1]–[4]. In adults, the normal pulse rate is 60-100 beats/min. Meanwhile, the abnormal pulse rate is <45 beats/min and >130 beats/min. For adults, the normal respiratory rate is 12-20 breaths/min. While the abnormal respiratory rate is <10 breaths/min and >26

breaths/min[5]–[7]. Vital signs play a crucial role in monitoring the progress of adult or pediatric patients during hospitalization, as they enable prompt detection of delayed recovery or adverse events. Vital signs are measured to obtain fundamental indicators of the patient's health status. The measurement of vital signs, including blood pressure, temperature, pulse, and respiratory rate, is the most common intervention in hospital medicine. Advanced monitoring systems combine clinical and technological aspects to deliver innovative healthcare outcomes. Remote patient monitoring systems are increasingly becoming the cornerstone of healthcare delivery, replacing traditional manual recording

with computer and smartphone-based electronic recording as a versatile and innovative health monitoring system. This study aims to design a Vital Sign Monitoring Parameter BPM and RR tool with Notifications via the IoT-Based Telegram application. The tool enables the monitoring of vital signs, particularly BPM and RR, regardless of the patient's location and at any given time. This allows doctors, health workers, and patients to stay informed about their health conditions. Real-time display of vital sign data is available through the TFT LCD screen, and the data from the screen can be accessed via Telegram. The Telegram application will send notifications in the event of abnormal patient conditions. MAX30100, a digital sensor for detecting breathing rate and heart rate, is utilized in this research. Furthermore, the data obtained shows errors that are within the allowable limits for each parameter.

In a previous study, Anggi Zafia made a prototype of an Inpatient Vital Monitoring Device using a Wireless Sensor as a Physical Distancing Effort for handling Covid 19 using Zigbee [8]. A similar study was also conducted by Fahmi Farisandi and Ahmad Fatkudin on Portable Patient Diagnostics equipped with Normal/Abnormal Indicators [9]. The device analyzed the rate of change of BPM and changes in the patient's body temperature. Several researchers and manufacturing companies in the medical field were conducting research and development of this system used for daily heart activity monitoring needs, as was done by [6] using the Max30100 sensor and Arduino microcontroller with a personal computer display with an accuracy of 92.36%. However, this system will only output BPM (Beat Per Minute) data. The other research [10] was a heart rate monitor based on a laptop interface microcontroller, using an AD8232 sensor and an Arduino Nano microcontroller, displaying ECG waveforms, bpm counts, and images of normal heart rates [11]–[13]. Some of these studies used laptop displays, which are inflexible for some users.

Therefore, we need a device design that can be used easily in monitoring heart rate using a PC or smartphone display at a low cost. The recording results can be known directly, then stored in a WEB application sent via internet media, known as IoT-based. The use of IoT systems in the medical world can also facilitate the information system[14]. Anan Wongjan, Amphawan Julsereewong, and Prasit Julsereewong made a device to measure heart rate and oxygen saturation in real-time using two LEDs, namely a red LED and an infrared LED, as well as a photodiode. The photodiode used is TCS-230 which is used to detect the intensity of light on the two LEDs reflected by the finger veins. To be able to produce readings of heart rate and oxygen saturation, this device is used on the finger. The measurement signal is processed using LabVIEW, which displays real-time heart rate per minute (BPM) and oxygen saturation readings. This device also has a probe-off alarm

and a warning message when the finger is not attached to the sensor [1][15]. In this study, the machine had a fairly large shape besides that sensor readings are sent to a computer via NI_USB-6009, a data acquisition module, so it was not easy to carry anywhere, and wireless communication with Bluetooth is not yet supported. A 2019 study, heart rate monitoring and oxygen saturation through smartphones was created by Arys Sulisty Utomo et al. from the Electrical Engineering Academy, made to monitor heart rate and oxygen saturation that can be monitored via a smartphone [16]. The drawback of this study was the readings of the heart rate and oxygen saturation values were different between the display on the LCD and the smartphone due to the unequal time of sending the reading data. In the same year, research was conducted on a Hypoxic Symptom Detection System Based on Oxygen Saturation and Heart Using the Arduino-Based Fuzzy Method by Dian Bagas Setyo Budi et al. from Brawijaya University [17]. In 2013, Yessy Mega Jayanti made a Portable BPM With a Finger Sensor Based on the ATtiny2313 Microcontroller[18]; there were shortcomings in this study because this device did not have a remote monitor and RTC to find outpatient data every hour. Then it was developed by Riszqy Cahyaning Maulina, who made a Heart Rate Monitoring device with a Graphic LCD equipped with an SD Card and RTC storage[19][20]. However, the drawback of this device was that its physical condition was still large and did not display BPM but instead displayed a graph. Fachrul Rozie from Electrical Engineering, Tanjungpura University, in 2016, developed previous research with his research, namely the design of an android-based heart rate monitoring device[21]. However, the drawback of this device is that it only has one parameter. Guruh Hariyanto, Universitas Airlangga, continued his research, designing a digital oximeter based on the Atmega16 microcontroller, and found a drawback: the device only uses one parameter and is not portable[22]. In 2017, Lokeswara Darmalaksana, with his research, was a portable BPM with a finger sensor equipped with RTC and SD card storage[22]. In 2019, Sofiyah made a Measuring Respiration Rate Via Android.[23] The objective of the study is to design a respiration rate monitor via an Android mobile phone. In this study, we used flex sensors to detect the respiration rate. The flex sensors[24][25] were placed in the human stomach diaphragm which detects changes in the human stomach diaphragm during breathing. The measurement results are displayed on the liquid crystal display (LCD) 2 x 16. [26][27][28] In 2022, Elga Rahmah Ramadhani1 made a Vital Signs Monitoring Device with BPM and SpO2 notifications using the Telegram Application Based on the Thingier.io Platform [1]. There are drawbacks in this study because this tool cannot display parameter value data on telegrams and settings for selecting patients on the tool [29]. Based on the literature search that has been described, the

author wants to create an "IoT-Based Human Vital Sign Monitoring Tool Using Telegram Notifications (BPM Parameters and Respiration Rate).

II. MATERIALS & METHOD

This A. EXPERIMENTAL SETUP The study used data capture at 8 points in the media incubator laboratory with temperatures at 35°C and 37°C and compare between Standards and the manufacturer's thermometer.

1) MATERIALS AND TOOLS

This study uses MAX30100 and DS18B20 finger sensors as signal amplifiers, and the microcontrollers used are Arduino Mega and esp32 as data senders[30].

2) EXPERIMENTS

In this study, after the design was completed, the design was tested using a media patient monitor and compared with a data logger whose results from the design were displayed by an Android phone at each measurement point.

3. THE BLOCK DIAGRAM

on the tool that will display the BPM parameters and Respiration Rate using the MAX30100 sensor module which is then processed by the ESP32 microcontroller with the output displayed on the TFT LCD and Smartphone on the Telegram application

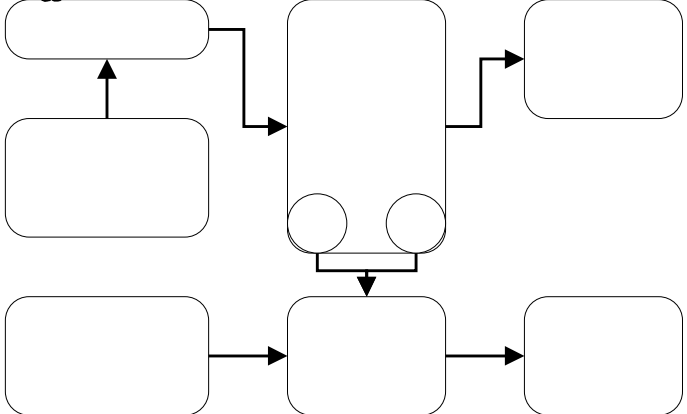


FIGURE 1. block diagram

3. THE FLOWCHART

MAX30100 sensor as input for [31]. Input that has been detected will be received and processed in the ESP32 microcontroller as the controller of the circuit. The output of the data generated by the microcontroller is in the form of values and signals from BPM and RR which will be displayed on the TFT LCD and Smartphone with Telegram notifications. When the tool is turned on, the initialization process will occur. The BPM circuit will detect the BPM signal. If a BPM signal is detected, the program will process the BPM signal data. Then Bluetooth version 4.2 ESP32 will send BPM signal data and receive heart rate values. Then from ESP32 the data will be sent and processed on the Smartphone via the telegram application. Smartphone with

Telegram notifications turned on, the initialization process will occur. The BPM circuit will detect the BPM signal. If a BPM signal is detected, the program will process the BPM signal data. Then Bluetooth version 4.2 ESP32 will send BPM signal data and receive heart rate values. Then from ESP32 the data will be sent and processed on the Smartphone via the telegram application.

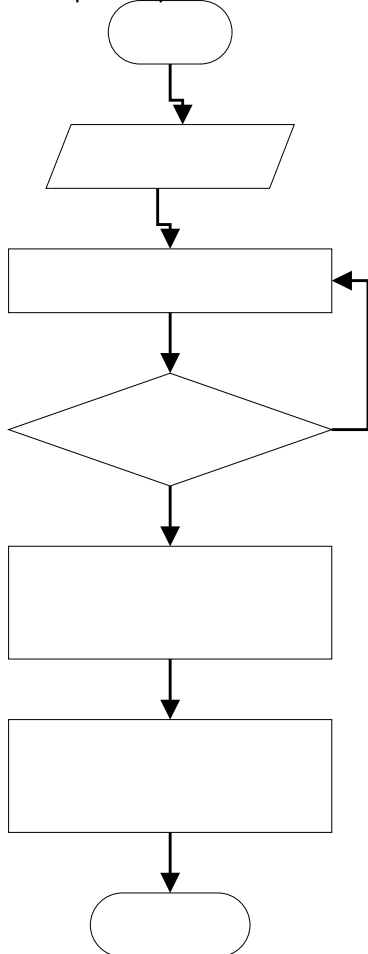


FIGURE 2. The system flowchart

A. DATA ANALYSIS

Measurement of each parameter BPM and RR, with multiplexer settings 1, 4, 7, and 10 seconds. everything is repeated 5 times. The average value of the measurement is obtained by using the mean or the average by applying equation (1). The average is the number obtained by dividing the number of values by the number of data in the set.:

(1)

where x denotes the mean (mean) for the n-measurements, x1 denotes the first measurement, x2 denotes the second measurement, and xn denotes measurementn95ts. Standard deviation is a value that indicates the degree (degree) of variation in a data set or a measure of the standard deviation of the mean. The

standard deviation (SD) formula can be shown in the equation (2):

where xi indicates the number of desired values, \bar{x} indicates the average of the measurement results, and n indicates the number of measurements. Uncertainty (UA) is a doubt that appears in each measurement result[32][33][34]. The uncertainty formula is shown in the equation (3):

where UA indicates the uncertainty value of the total measurement, SD indicates the resulting standard deviation, and n indicates the number of measurements. %error indicates a system error. The lower Error value is the average difference of each data. Errors can indicate deviations between the standard and the design or model. The error formula is shown in the equation (4).

where xn is the measured value of the machine calibrator. X is the measured value of the design.

III. RESULT

In this study, the module has been tested using a comparison tool Oximeter and Thermogun. FIGURE 3 and FIGURE 4 are a microcontroller circuit consisting of a Wemos D1 Mini, a battery circuit, an envelope, and an amplifier circuit. The power supply circuit is made using a Lithium Battery which will enter the voltage-up module.

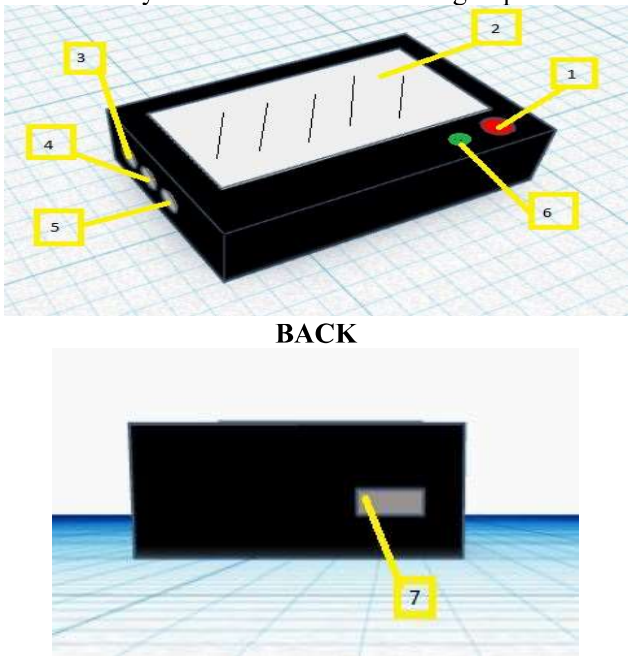


FIGURE 3 . Device monitoring

The digital part consists of the Wemos D1 Mini microcontroller which is the main board of the device the SEN0203 BPM sensor, and the MLX90614 temperature

sensor. The process of collecting data on the module is carried out at RSUD Dr. Mohamad Saleh Probolinggo City. The data retrieval process was carried out on the 1st, 4th, 7th, and 10th-second multiplexer for 5 experiments using the BPM sensor SEN0203 and the MLX90614 Temperature sensor.



FIGURE 4 . pengambilan data

| TABLE 1 Error value for each multiplexer setting in comparison of module values with oximeter and thermogun comparison tools | |
|--|-------|
| Respondent | Error |
| 1 | 1,8% |
| 2 | 0,8% |
| 3 | 1,7% |
| 4 | 0,6 |
| 5 | 0,8 |
| Rata-rata | 1,14% |

Error is the difference from the actual value compared to the measured value of the module with units in this study, namely BPM for heart rate, and C for temperature units. It can be seen in TABLE 1 that Measurements were taken on 5 respondents, and each respondent was measured 10 times which was then averaged. From the results of these data measurements, the results obtained were different from the average measurement of the comparison device, namely the patient monitor. The biggest difference value from the respondent's measurement is 1.2%. The average measurement is 1.14%.

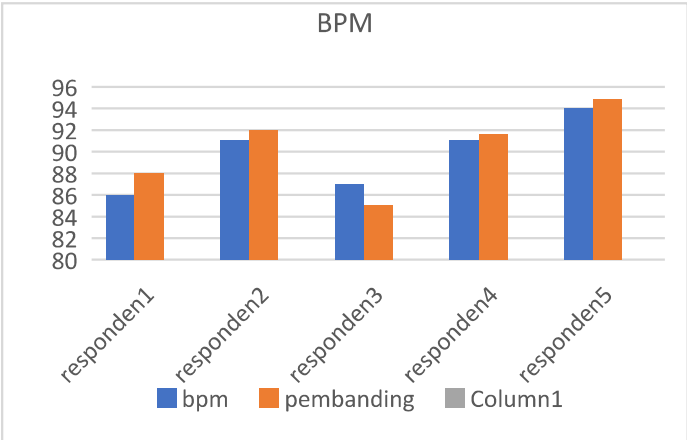


FIGURE 5. Graph of the error value of each set in the comparison of the value of the High Flow Oxygen Analyzer module with the Citrex H3 comparison tool (green: BPM and blue: temperature).

Based on the measurement results of the respondents, the measurement results were found to be within the tolerance range. This measurement was carried out on 5 respondents with 10 measurements. The results of the measurement of the BPM module are compared with the tools on the market, namely the Pulse Oximeter by looking at the BPM value. 80 90 100 BPM Comparison Oximeter (BPM).

TABLE 2
Comparison of standard deviation values for each multiplexer setting on the comparison of module values with comparison tools oximeter and thermogun

| Respondent | Error |
|------------|-------|
| 1 | 0,8% |
| 2 | 0,8% |
| 3 | 0,8% |
| 4 | 0,9% |
| 5 | 0,9% |
| Rata-rata | 0,84% |

It can be seen from TABLE 2 that Measurements were taken on 5 respondents, and each respondent was measured 10 times which was then averaged. From the results of these data measurements, the results obtained were different from the average measurement of the comparison device, namely the patient monitor. The biggest difference value from the respondent's measurement is 0.1%. The average measurement is 0.84%.

IV. DISCUSSION

Based on the results of the discussion and the purpose of making modules, monitoring patient progress, both inpatient cases and children for vital signs indicators can be easily determined the patient's health status, therefore making modules for BPM and RR known through the Telegram application and TFT LCD screen is a form of development of this research. This module also uses a microcontroller, namely ESP32 whose specifications are more adequate for delivery on the Telegram application. In

addition, the measurement of BPM and RR parameters with a comparison was carried out by 5 respondents and 10 measurements. The BPM data taken has an average error value of 0.66% and the RR data taken has an average error value of 1.8% while there are still many weaknesses in this tool. If the finger position does not match, the reading will be unstable and inaccurate.

IV. CONCLUSION

The conclusion of the results of this research discussion can lead to the development of modules that allow doctors, health workers, and patients to stay informed about their health conditions. Real-time display of vital signs is available through the TFT LCD screen, and Telegram so that with this Telegram Application will send notifications if an abnormal patient condition occurs. Furthermore, this module still has problems about sensor readings, especially in reading respiratory rate parameters.

REFERENCES

S. Luthfiyah, E. R. Ramadhani, T. B. Indrato, A. Wongjan, and K. O. Lawal, "Vital Signs Monitoring Device with BPM and SpO2 Notification Using Telegram Application Based on Thinger.io Platform," *Indonesian Journal of Electronics, Electromedical Engineering, and Medical Informatics*, vol. 4, no. 1, pp. 1–7, 2022, doi: 10.35882/ijeemi.v4i1.1.

H. Zahid *et al.*, "Portable Smart Mini Patient Monitor for Improved Healthcare Outcomes: Patient-Based Care Device," *Pakistan Journal of Science*, vol. 73, no. 1, pp. 88–95, 2021.

M. Harford, J. Catherall, S. Gerry, J. D. Young, and P. Watkinson, "Availability and performance of image-based, non-contact methods of monitoring heart rate, blood pressure, respiratory rate, and oxygen saturation: A systematic review," *Physiological Measurement*, vol. 40, no. 6, 2019, doi: 10.1088/1361-6579/ab1f1d.

Z. Ar, O. Al, and A. Ap, "COVID-19 pandemic management: a multi-parameter portable healthcare monitoring device," *International Journal of Biosensors & Bioelectronics Research*, vol. 7, no. November, pp. 116–120, 2021, doi: 10.15406/ijbsbe.2021.07.00224.

J. Gleichauf *et al.*, "Automated non-contact respiratory rate monitoring of neonates based on synchronous evaluation of a 3d time-of-flight camera and a microwave interferometric radar sensor," *Sensors*, vol. 21, no. 9, 2021, doi: 10.3390/s21092959.

I. Wheatley, "Respiratory rate 5: using this vital sign to detect deterioration," *Nursing Times*, vol. 114, no. 10, pp. 45–46, 2018.

A. R. Zizzo, I. Kirkegaard, J. Hansen, N. Uldbjerg, and H. Mølgaard, "Fetal Heart Rate Variability Is Affected by Fetal Movements: A Systematic Review," *Frontiers in Physiology*, vol. 11, no. September, 2020, doi: 10.3389/fphys.2020.578898.

Izhangghani, I. Hikmah, and Slamet Indriyanto, "Prototype of Body Temperature and Oxygen Saturation Monitoring System Using DS18B20 and MAX30100 Sensors based on IOT," *Jurnal RESTI (Rekayasa Sistem dan Teknologi Informasi)*, vol. 6, no. 5, pp. 810–817, 2022, doi: 10.29207/resti.v6i5.4385.

R. Austin, F. Lobo, and S. Rajaguru, "GSM and Arduino Based Vital Sign Monitoring System," *The Open Biomedical Engineering Journal*, vol. 15, no. 1, pp. 78–89, 2021, doi: 10.2174/1874120702115010078.

Q. N. Alsahi, A. F. Marhoon, and A. H. Hamad, "Remote Patient Healthcare surveillance system based real-time vital signs," *Al-Khwarizmi Engineering Journal*, vol. 16, no. 4, pp. 41–51, 2020, doi: 10.22153/kej.2020.10.003.

N. Wessel, M. Riedl, and J. Kurths, "Is the normal heart rate 'chaotic' due to respiration?," *Chaos*, vol. 19, no. 2, 2009, doi: 10.1063/1.3133128.

S. P. von Steinburg *et al.*, "What is the 'normal' fetal heart rate?," *PeerJ*, vol. 2013, no. 1, 2013, doi: 10.7717/peerj.82.

Bahar Gholipour and Nicoletta Lanese, "What is a normal heart rate?," <https://www.livescience.com/42081-normal-heart-rate.html>.

[14] F. Aktas, C. Ceken, and Y. E. Erdemli, “IoT-Based Healthcare Framework for Biomedical Applications,” *Journal of Medical and Biological Engineering*, vol. 38, no. 6, pp. 966–979, 2018, doi: 10.1007/s40846-017-0349-7.

[15] A. Wongjan, A. Julsereewong, and P. Julsereewong, “Continuous Measurements of ECG and SpO₂ for Cardiology Information System,” *MultiConference of Engineers and Computer Scientists*, vol. II, pp. 18–21, 2009.

[16] A. Nemcova *et al.*, “Monitoring of heart rate, blood oxygen saturation, blood pressure using a smartphone,” *Biomedical Signal Processing and Control*, vol. 59, p. 101928, 2020, doi: 10.1016/j.bspc.2020.101928.

[17] S. Mayya, V. Jilla, V. N. Tiwari, M. M. Nayak, and R. Narayanan, “Continuous monitoring of stress on smartphone using heart rate variability,” *2015 IEEE 15th International Conference on Bioinformatics and Bioengineering, BIBE 2015*, no. c, 2015, doi: 10.1109/BIBE.2015.7367627.

[18] B. De Ridder, B. Van Rompaey, J. K. Kampen, S. Haine, and T. Dilles, “Smartphone Apps Using Photoplethysmography for Heart Rate Monitoring: Meta-Analysis,” *JMIR Cardio*, vol. 2, no. 1, 2018, doi: 10.2196/cardio.8802.

[19] A. S. Utomo, E. H. P. Negoro, and M. Sofie, “Monitoring Heart Rate Dan Saturasi Oksigen Melalui Smartphone,” *Simetris: Jurnal Teknik Mesin, Elektro dan Ilmu Komputer*, vol. 10, no. 1, pp. 319–324, 2019, doi: 10.24176/simet.v10i1.3024.

[20] C.-L. Ho, Y.-C. Fu, M.-C. Lin, S.-C. Chan, B. Hwang, and S.-L. Jan, “Smartphone Applications (Apps) for Heart Rate Measurement in Children: Comparison with Electrocardiography Monitor,” *Pediatric Cardiology*, vol. 35, no. 4, pp. 726–731, 2014, doi: 10.1007/s00246-013-0844-8.

[21] J. Turner, C. Zellner, T. Khan, and K. Yelamarthi, “Continuous heart rate monitoring using smartphone,” *IEEE International Conference on Electro Information Technology*, pp. 324–326, 2017, doi: 10.1109/EIT.2017.8053379.

[22] R. B. Lagido, J. Lobo, S. Leite, C. Sousa, L. Ferreira, and J. Silva-Cardoso, “Using the smartphone camera to monitor heart rate and rhythm in heart failure patients,” *2014 IEEE-EMBS International Conference on Biomedical and Health Informatics, BHI 2014*, pp. 556–559, 2014, doi: 10.1109/BHI.2014.6864425.

[23] S. Shofiyah, I. D. G. Hari Wisana, T. Triwiyanto, and S. Luthfiyah, “Measuring Respiration Rate Via Android,” *Indonesian Journal of electronics, electromedical engineering, and medical informatics*, vol. 1, no. 1, pp. 20–26, 2019, doi: 10.35882/ijeemi.v1i1.4.

[24] M. Hernandez-Silveira *et al.*, “Assessment of the feasibility of an ultra-low power, wireless digital patch for the continuous ambulatory monitoring of vital signs,” *BMJ Open*, vol. 5, no. 5, pp. 1–9, 2015, doi: 10.1136/bmjopen-2014-006606.

[25] P. S. Das *et al.*, “A Wearable Multisensor Patch for Breathing Pattern Recognition,” vol. 23, no. 10, pp. 10924–10934, 2023, doi: 10.1109/JSEN.2023.3264942.

[26] G. Cinel, “Wearable respiratory rate sensor technology for diagnosis of sleep apnea”.

[27] A. J. Puspitasari, D. Famella, M. Sulthonur Ridwan, and M. Khoiri, “Design of low-flow oxygen monitor and control system for respiration and SpO₂ rates optimization,” *Journal of Physics: Conference Series*, vol. 1436, no. 1, 2020, doi: 10.1088/1742-6596/1436/1/012042.

[28] N. Hayward *et al.*, “A capaciflector provides continuous and accurate respiratory rate monitoring for patients at rest and during exercise,” *Journal of Clinical Monitoring and Computing*, vol. 36, no. 5, pp. 1535–1546, 2022, doi: 10.1007/s10877-021-00798-7.

[29] S. Luthfiyah, E. R. Ramadhani, T. B. Indrato, A. Wongjan, and K. O. Lawal, “Vital Signs Monitoring Device with BPM and SpO₂ Notification Using Telegram Application Based on Thingier.io Platform,” *Indonesian Journal of Electronics, Electromedical Engineering, and Medical Informatics*, vol. 4, no. 1, 2022, doi: 10.35882/ijeemi.v4i1.1.

[30] Muhammad Nur Fariz and Jamaaluddin, “Design for Monitoring Blood Pressure, Non-Invasive Blood Sugar, Weight, and Body Temperature Based on Internet of Things,” *Procedia of Engineering and Life Science*, vol. 1, no. 1, 2021, doi: 10.21070/pels.v1i1.814.

[31] N. Mohammadi-Koushki, H. Memarzadeh-Tehran, and S. Goliaei, “A Wearable Device for Continuous Cardiorespiratory System Monitoring,” in *Proceedings - Conference on Local Computer Networks, LCN*, 2016. doi: 10.1109/LCN.2016.052.

A. Rahman *et al.*, “Towards health monitoring using remote heart rate measurement using digital camera: A feasibility study,” *Measurement: Journal of the International Measurement Confederation*, vol. 8, no. 2, pp. 1–7, 2019, doi: 10.21107/triac.v4i2.3257.

A. R. Zizzo, I. Kirkegaard, J. Hansen, N. Uldbjerg, and H. Mølgaard, “Fetal Heart Rate Variability Is Affected by Fetal Movements: A Systematic Review,” *Frontiers in Physiology*, vol. 11, no. September, 2020, doi: 10.3389/fphys.2020.578898.

M. A. Hassan, A. S. Malik, D. Fofi, B. Karasfi, and F. Meriaudeau, “Towards health monitoring using remote heart rate measurement using digital camera: A feasibility study,” *Measurement: Journal of the International Measurement Confederation*, vol. 149, p. 106804, 2020, doi: 10.1016/j.measurement.2019.07.032.